




MASS SPECTROMETRY REPORT

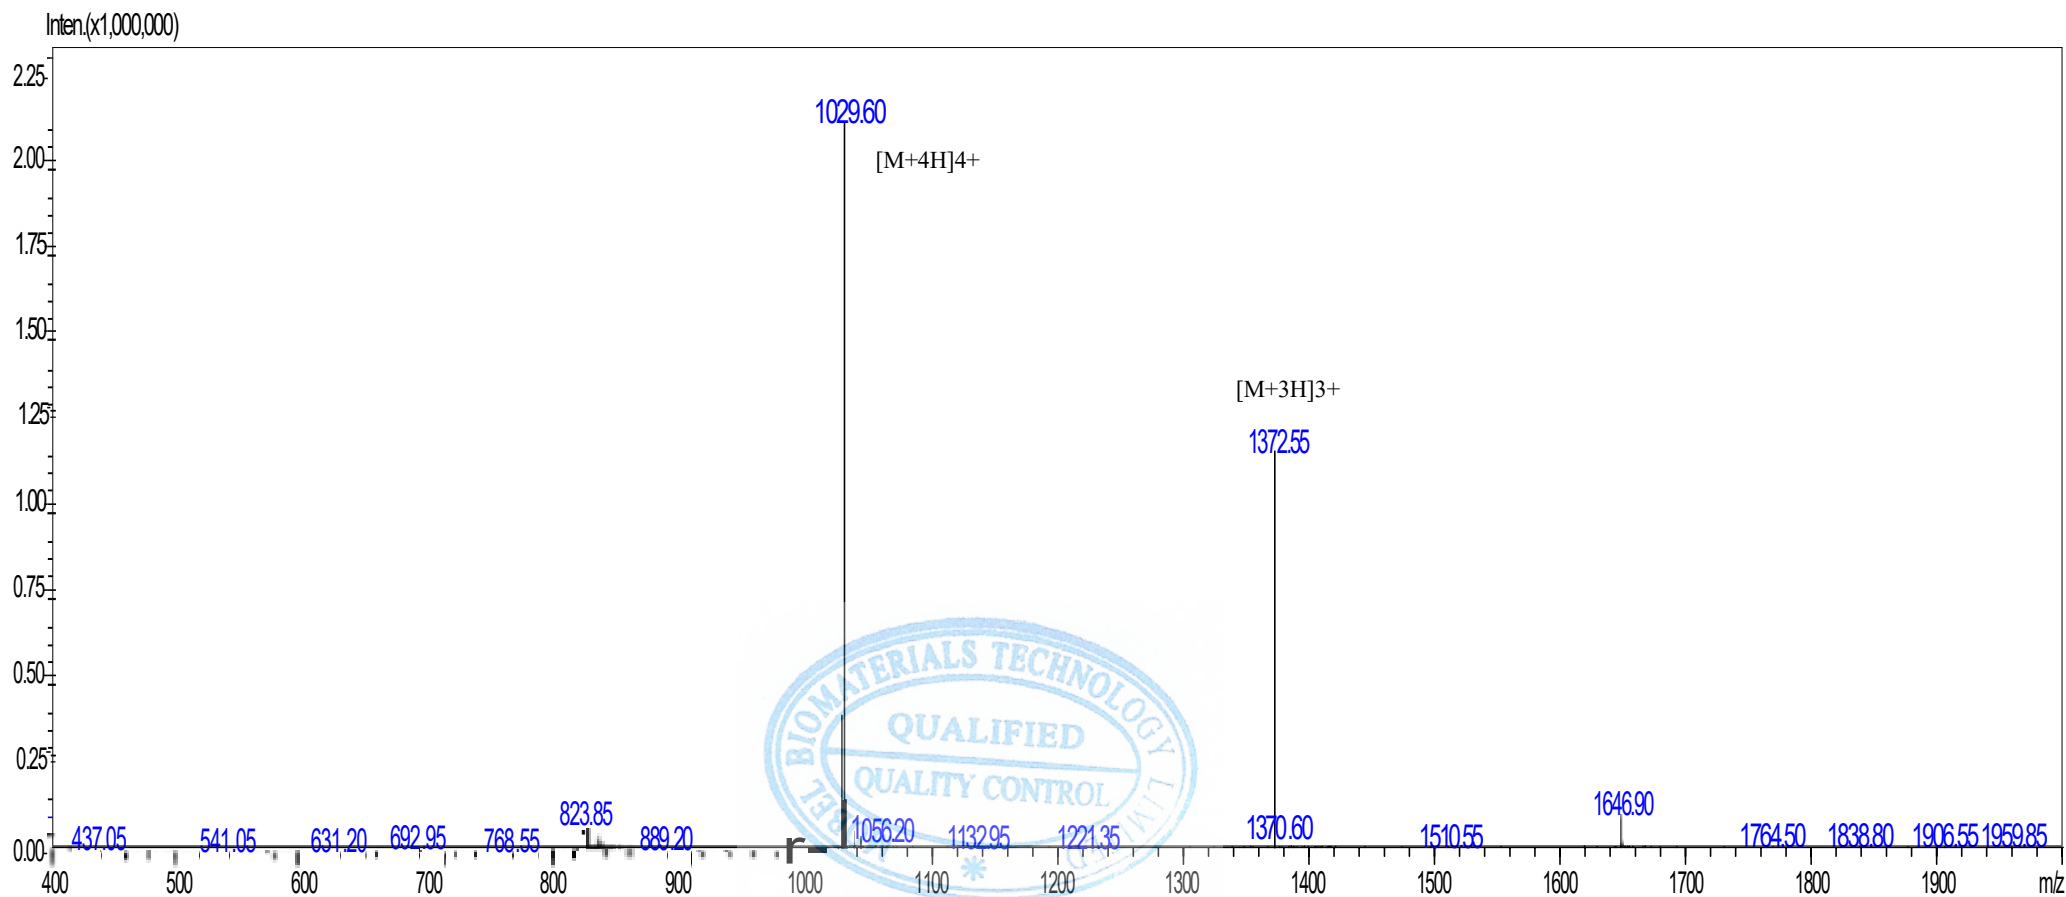

Sample Description

Analyzed date: 2025-01-13
Analyst: Yan.li
Sample: SGPT-MB250113
M.W.: 4113.6
Lot. No.: SGPT-MB50113

Instrument

Probe:
Nebulizer Gas Flow:
CDL:
CDL Temp.:
Block Temp.:

SHIMADZU LCMS-2020

ESI
1.5L/min
-20.0v
250 °C
200 °C
Probe Bias: +4.5 kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H₂O/50%ACN